

TEST REPORT

(Electronic version)

扫码下载报告



No: 200076570

VERIFICATION WEBSITE: www.gtgc.net.cn

VERIFICATION CODE: JTNH-7018-14

ISSUE DATE 签发日期: 2020-05-03

APPLICANT: CareAble Biotechnology Co., Ltd
委托单位: 伏羲生物科技(广东)有限公司
ADDRESS: Building 0, Yekeng Industrial Area, Jiangmen City, Guangdong China
地址: 江门市宏兴路3号0幢(自编002)

INFORMATION CONFIRMED BY APPLICANT 客户认定信息:

KN95 FILTRATION RESPIRATORS 一次性KN95防护口罩 35个
SIZE 号型规格: CARE002

DATE RECEIVED/DATE TEST STARTED: 2020-04-13

样品受理/测试开始日期: 2020-04-13

CONCLUSION 结论:

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER NaCl颗粒物过滤效率	M
INSPIRATORY RESISTANCE 吸气阻力	M
EXPIRATORY RESISTANCE 呼气阻力	M

NOTE: "M" - MEET THE STANDARD'S REQUIREMENT "F" - FAIL TO MEET THE STANDARD'S REQUIREMENT

"—" - NO COMMENT

备注: "M" - 符合标准要求 "F" - 不符合标准要求

"—" - 此项目不判定

REMARK:

ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).

本报告中检验检测项目均在相应标准规定的环境条件下进行(有注明的除外)。

COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.

复印件、副本未重新加盖报告书确认章无效。

THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

本报告检验检测地址为广州市番禺区珠江路1号。

APPROVED BY(签发):

刘圆 工程师

Yuan Liu ENGINEER


刘圆



TEST REPORT

(Electronic version)

No:200076570

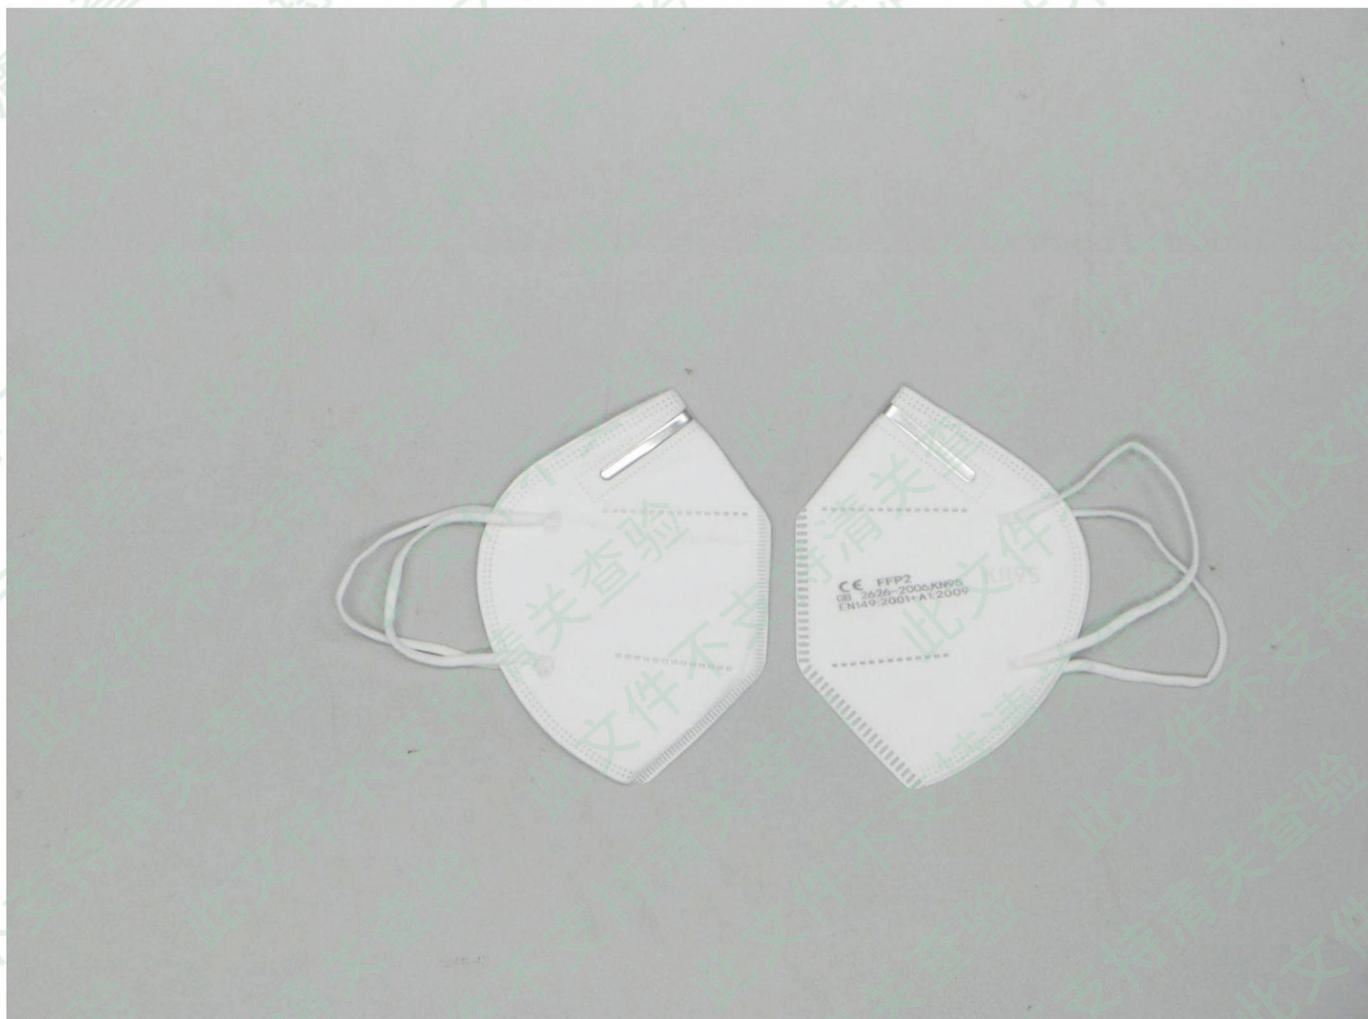

TEST REPORT

(Electronic version)

No:200076570

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER (%) NaCl颗粒物过滤效率(%)

(GB 2626-2006 6.3, AIR FLOW 空气流量:85L/min, AEROSOL 气溶胶颗粒:NaCl, AEROSOL
CONCENTRATION 气溶胶浓度, 15mg/m³, TEMP 温度:23.7℃ RH 湿度:35.4%)

FILTRATION EFFICIENCY 过滤效率:
UNTREATED SAMPLE 未处理样品

1# 99.363
2# 99.466
3# 99.382
4# 99.420
5# 99.499
6# 99.210
7# 99.215
8# 99.153
9# 99.352
10# 99.461

REQUIREMENT 要求
FILTRATION EFFICIENCY 过滤效率:
≥95.0
(KN95)
(GB 2626-2006)

CONDITIONING TREATED 温湿度预处理后样品

1# 98.53
2# 98.60
3# 98.47
4# 98.67
5# 98.89

INSPIRATORY RESISTANCE (Pa) 吸气阻力(Pa)

(GB 2626-2006 6.5, HEAD SIZE 头模: MEDIUM 中号)

UNTREATED SAMPLE 未处理样品:

1# 146.6
2# 140.9

PRETREATMENT SAMPLE 预处理样品:

1# 136.6
2# 133.7

REQUIREMENT 要求
≤350
(GB 2626-2006)

EXPIRATORY RESISTANCE (Pa) 呼气阻力(Pa)

(GB 2626-2006 6.6, HEAD SIZE 头模: MEDIUM 中号)

UNTREATED SAMPLE 未处理样品:

1# 139.6
2# 132.2

PRETREATMENT SAMPLE 预处理样品:

1# 124.1
2# 121.8

REQUIREMENT 要求
≤250
(GB 2626-2006)



——本报告结束(End of Report)——

PAGE 3 OF 3